
	<b>CSA: Simian Panel A</b> (Product Number 12-1212) <b>User Protocol</b>	<b>Literature Number</b>  <b>L756 27June2018</b>	<b>Page</b>  <b>1 of 9</b>
---	--	--	----------------------------------

## Table of Contents

---

1.0	Introduction.....	2
2.0	Kit Contents.....	3
3.0	Required Materials.....	3
4.0	Storage.....	3
5.0	Safety and Handling.....	4
6.0	Protocol Overview.....	4
7.0	Procedure.....	4
8.0	Ordering Information.....	8
9.0	Appendix A: Troubleshooting.....	9

**NOTE: FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC USE.** The information presented in this document is for suggested use only; the product is offered without any warranty or guarantee due to the variability in final use conditions and material handling by the user. No claims beyond replacement of unacceptable material or refund of purchase price shall be allowed.

	<b>CSA: Simian Panel A</b> (Product Number 12-1212) <b>User Protocol</b>	<b>Literature Number</b>  <b>L756 27June2018</b>	<b>Page</b>  2 of 9
---	--	--	---------------------------

## 1.0 Introduction

### 1.1 CSA: Simian Panel A Overview


The health and well-being of your non-human primate (NHP) colonies are critical to the success of your research. The Colony Surveillance Assay™: Simian Panel A assay can provide a sensitive, robust and user-friendly alternative to ELISA or bead-based methods by combining multiplex detection technologies with compact and cost-effective analysis tools for colony health screening. This approach provides an indication of previous exposure to pathogenic agents present in NHP colonies, both to identify potential infectious threats to the colony and their human caretakers and to ensure your research remains uncompromised.


The CSA: Simian Panel A is intended to be used as a tool for the continual monitoring of your specific pathogen-free (SPF) colony. This method measures specific serum IgG in a multiplex format, providing you with data for tracking your colony's health. The use of CSA: Simian Panel A kit is intended for use as a profiling assay and not a definitive diagnostic assay. Cut-off values have been determined through robust validation methods to provide universal optimal sensitivity, and are to be used as suggested starting points for your analysis. Routine surveillance of your colony with the CSA: Simian Panel A assay will give you confidence in your colony health, and reduce the number of samples needing to be tested by more expensive and time-consuming methods.

**NOTE:** Intuitive Biosciences highly recommends using secondary methods (such as IFA or PCR) to validate your results, resolve equivocal results, and confirm positive results in your SPF colony.

The CSA: Simian Panel A kit consists of reagents sufficient to process up to ninety-two samples, and the included control sera. The CSA: Simian Panel A kit uses the same basic laboratory instruments as an ELISA. The SilverQuant® chromogenic reagents are used for signal generation on the CSA: Simian products. Assay results are measured using the AthenaQuant® System, where data is easily generated using a scanner and quickly analyzed using the included AthenaQuant software.

**Figure 1. CSA: Simian Panel A Schematic**

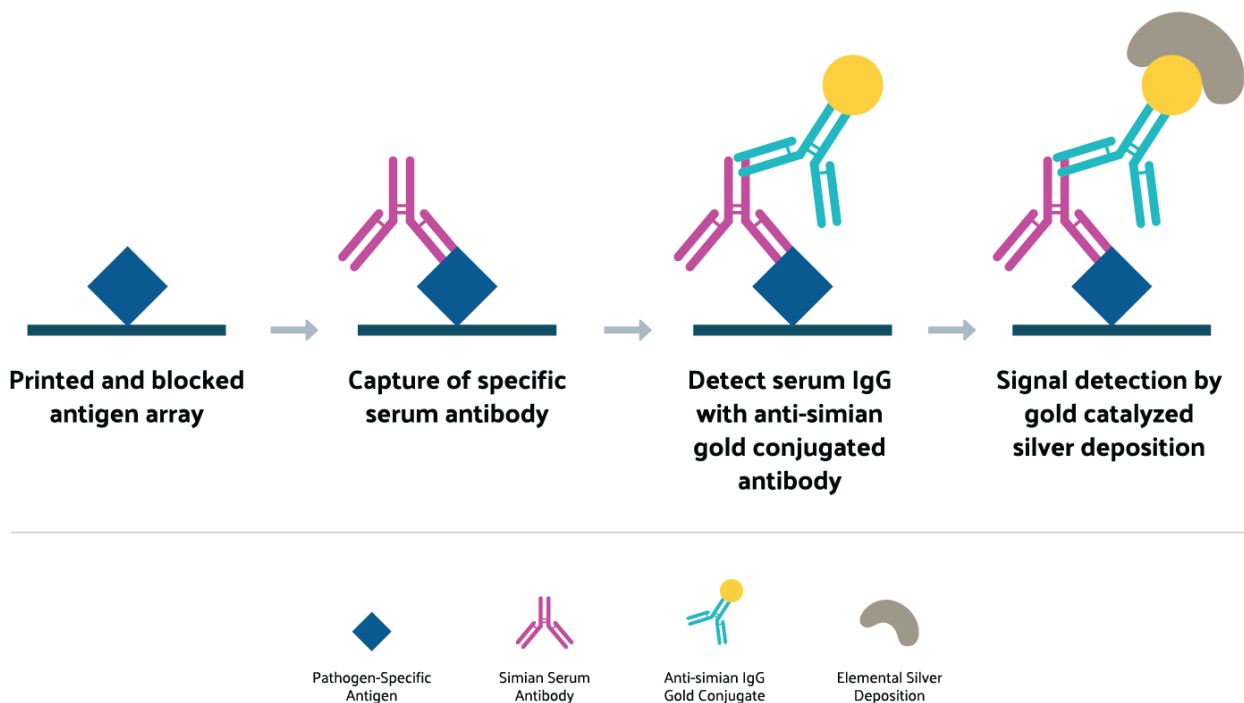

	<b>CSA: Simian Panel A</b> (Product Number 12-1212) <b>User Protocol</b>	<b>Literature Number</b>  <b>L756 27June2018</b>	<b>Page</b>  3 of 9
---	--	--	---------------------------

## 1.2 SilverQuant Surface Chemistry

The CSA: Simian Panel A arrays are printed on Intuitive Biosciences' proprietary protein plates and are specifically designed for multiplex immunoassays and deliver high signal-to-noise with high sensitivity for protein microarray applications.

## 2.0 Kit Contents


Component	Description	Quantity	Prod. No.
CSA: Simian Panel A Plate	Plate containing 96 wells consisting of antigens representing unique simian pathogens	1 plate	12-1210
5X Slide Wash Buffer	Buffer used to remove unbound protein	100 mL	2-1039
CSA Buffer	Buffer used to dilute samples and Gold Detection Reagent	100 mL	7-1037
Positive Control	Positive control sample	10 µL	12-1049
Negative Control	Negative control sample	10 µL	12-1009
SilverQuant Anti-simian IgG Gold Conjugate	Gold Detection Reagent	100 µL	10-2139
SilverQuant Reagent A	Development Reagent A	10 mL	10-2132
SilverQuant Reagent B	Development Reagent B	10 mL	10-2112
Plate™ Well Seals	Used to seal wells during sample incubation	1 each	4-1009
96 Deep Well Dilution Plate	Used for serum dilutions	1 each	12-1025
CSA: Simian Panel A Plate User Protocol			L756

## 3.0 Required Materials

Component	Description
Bench-top microcentrifuge	Capacity to hold 1.5 mL microcentrifuge tubes
Vortex Mixer	Various
1.5 mL Microcentrifuge tubes	Various
15 mL conical tubes	Various
50 mL conical tubes	Various
Deionized or Ultrapure Water	Clean water
Microarray Scanner	AQ 1000
Microarray Image Analysis Software	AthenaQuant software (included with Product AQ 1000)
CSA: Simian Panel A data analysis template	Included with AthenaQuant software
Micropipettes	Single, Repeat, and 8-channel; various capacities

## 4.0 Storage

The CSA: Simian Panel A (Prod. No. 12-1212) kit should be stored at 2-8°C until used.

	<p align="center"><b>CSA: Simian Panel A</b> (Product Number 12-1212) User Protocol</p>	<p align="center"><b>Literature Number</b>  L756 27June2018</p>	<p align="center"><b>Page</b>  4 of 9</p>
---	---	---	---

## 5.0 Safety and Handling

Use Universal Safety Precautions when handling animal body fluids. For all other materials, normal precautions exercised in handling laboratory materials should be followed. The material is not considered hazardous according to 29CFR1910.1200. The chemical, physical, and toxicological properties of this product may not, as yet, have been thoroughly investigated. We recommend the use of gloves, lab coats, and eye protection when working with any material.

## 6.0 Protocol Overview

The CSA: Simian Panel A kit contains sufficient reagents for qualitative analysis of up to 92 serum samples. However, only a single assay may be performed with the reagents included in the kit. Reagent B is air sensitive and once opened, it must be used within a day. Both Reagent A and Reagent B are light sensitive and should not be exposed to direct or excess light.

If desired partial plates can be run, but unopened Reagent A and Reagent B must be used. Additional reagents for regular use of partial plates are available.

CSA: Simian Panel A plates should be handled with care (never touch the bottom of the well) and not allowed to dry once they have been wetted. Proper storage and handling of serum samples is critical for obtaining optimal data. Avoid repeated freeze-thaw cycles and aliquot and freeze samples at -80°C for long-term storage.

Developed CSA array plates are stable and can be stored indefinitely at room temperature.

## 7.0 Procedure

### 7.1 Preparation of Buffers and Reagents


**NOTE:** Equilibrate entire kit to room temperature (18-30°C) prior to use for peak assay performance.

- 7.1.1 In a container capable of holding at least 500 mL, add 400 mL of ultrapure water. Add 100 mL of the 5X Slide Wash Buffer (Product No. 2-1039). Mix thoroughly. Store closed at room temperature for up to 1 month. Label as "1X Slide Wash Buffer".

### 7.2 Serum Dilution and Addition to the Array

**NOTE:** If using partial plate, cover the unused wells with plate seal (Prod. No. 4-1009) to make sure the wells will not be wetted at any time and can be used in the future.

**NOTE:** After step 7.2.3, do not allow the surface of the array to dry completely at any time before you are ready to scan the plate.

	<b>CSA: Simian Panel A</b> (Product Number 12-1212) <b>User Protocol</b>	<b>Literature Number</b>  <b>L756 27June2018</b>	<b>Page</b>  5 of 9
---	--	--	---------------------------

7.2.1 Note the location of each sample to be loaded in the plate map below.

	1	2	3	4	5	6	7	8	9	10	11	12
A	Positive Control											
B	Negative Control											
C												
D												
E												
F												
G												
H												

- 7.2.2 Ensure that each sample is completely thawed, and vortex briefly. Spin each sample at 5,000 rpm for at least 10 seconds to collect the material in the bottom of the tube.
- 7.2.3 Add 200  $\mu$ L of CSA Buffer (Product No. 7-1037) to each well of the CSA: Simian Panel A Plate (Product No. 12-1210) using a multi-channel pipettor. Tap the side of the Plate unit two times to ensure that the buffer covers each well completely.
- 7.2.4 Immediately remove the CSA Buffer from the wells by inverting over a sink or liquid disposal container three times. Remove excess solution from the top of the Plate by blotting dry with a lint-free wipe.
- 7.2.5 Using a multi-channel pipettor, immediately add 75  $\mu$ L of fresh CSA Buffer to each well, tap side of the Plate and set aside.
- 7.2.6 To the 96 Well Dilution Plate (Product No. 12-1025), pipette 500  $\mu$ L of CSA Buffer into all wells.
- 7.2.7 Add 5  $\mu$ L of Positive Control serum (12-1049) to well A1 (or the Positive Control well) of the 96-well dilution plate. Mix by pipetting up and down 3 times.
- 7.2.8 Add 5  $\mu$ L Negative Control (12-1009) to wells B1 (or the Negative Control well) of the 96-well dilution. Mix by pipetting up and down 3 times.
- 7.2.9 Add 5  $\mu$ L of each serum sample to be tested to remaining wells of the 96-well dilution plate as indicated in the table above. Mix by pipetting up and down 3 times.

**NOTE:** If your serum sample has been diluted, please adjust the dilution accordingly for a 1:100 dilution into the well dilution plate.

- 7.2.10 Set multichannel pipette to 25  $\mu$ L. For each column in the dilution plate, mix each sample by pipetting up and down 5 times prior to drawing up 25  $\mu$ L.
- 7.2.11 Dispense 25  $\mu$ L of diluted sample into each well of the CSA: Simian Panel A Plate (Prod. No. 12-1210), taking care not to touch the bottom of the well (pipette into a corner or side of the well).
- 7.2.12 Cover the wells with the provided plate seal (Prod. No. 4-1009) to prevent evaporation, tap side of the plate and incubate at room temperature for **1 hour**.
- 7.2.13 Discard sample dilution plate into appropriate biohazard waster container.

### 7.3 Wash 1 and Add Gold Conjugate Reagent


- 7.3.1 Briefly spin the SilverQuant Anti-Simian IgG Gold Conjugate (Product No. 10-2139) using a bench top microcentrifuge to collect all the material into the bottom of the tube and gently vortex to mix.
- 7.3.2 Prepare the Gold Conjugate Reagent by adding 96  $\mu$ L of SilverQuant Anti-Simian IgG Gold Conjugate to 12 mL of CSA Buffer. Mix gently and thoroughly.

**NOTE:** If using less than a full plate, adjust dilution volume accordingly. Final dilution of Anti-Simian IgG Gold is 1:125.

- 7.3.3 Remove the serum solutions from wells by covering the CSA: Simian Panel A Plate with a paper towel or other absorbent paper, invert, and, while holding the paper towel, tap down three times. Dispose of the adsorbent paper into a biohazardous waste container.
- 7.3.4 Add 200  $\mu$ L of 1X Slide Wash Buffer (SWB, prepared in **Step 7.1.1**) to each well using a repeat or multi-channel pipettor and tap side of the plate. Remove SWB by inverting plate over a liquid biohazard waste container.
- 7.3.5 Repeat step 7.3.4 two more times, adding 200  $\mu$ L of 1X Slide Wash Buffer for a total of 3 washes in the Plate.
- 7.3.6 Remove the final wash and immediately add 100  $\mu$ L Gold Conjugate Reagent (prepared in **Step 7.3.2**). Tap side of the plate to ensure bottom of the wells are completely covered.
- 7.3.7 Incubate for **1 hour** at room temperature.

### 7.4 Wash 2 and Development

- 7.4.1 Remove the Gold Conjugate Reagent from the CSA: Simian Panel A Plate inverting over a waste container. Shake plate firmly to remove liquid from bottom of wells.
- 7.4.2 Add 200  $\mu$ L of 1X Slide Wash Buffer to each well using a repeat or multi-channel pipettor. Tap side of plate. Remove Slide Wash Buffer by inverting plate over liquid waste.

	<b>CSA: Simian Panel A</b> (Product Number 12-1212) <b>User Protocol</b>	<b>Literature Number</b>  <b>L756 27June2018</b>	<b>Page</b>  7 of 9
---	--	--	---------------------------

7.4.3 Repeat **Step 7.4.2** two times, for a total of three washes. After final wash keep Slide Wash Buffer into wells until ready to perform **step 7.4.7**.

**NOTE:** SilverQuant Reagent A (Product No. 10-2132) and SilverQuant Reagent B (Product No. 10-2112) are sensitive to light. Be sure to perform the following steps out of direct sunlight.

It **CRITICAL** to add the reagent mix quickly to the CSA: Simian Panel A Plate because the reaction is time dependent. Once Reagent A and B have been mixed together and added to the reagent trough, quickly add to plate using a multi-channel pipettor or repeat pipettor.

Be sure to read and understand **Steps 7.4.4 -7.5.1** and have all the needed equipment prepared and ready.

7.4.4 Set a timer to 3 minutes.

7.4.5 Add pipet tips to a multichannel and prepare it to dispense 100  $\mu$ L. Obtain a fresh reagent trough capable of holding 20 mL of liquid.

7.4.6 Prepare the SilverQuant Development Reagent by directly pouring SilverQuant Reagent A (Product No. 10-2132) into SilverQuant Reagent B bottle (Product No. 10-2112). Cap the bottle and shake vigorously for ~3 seconds and pour into reagent trough.

7.4.7 Quickly remove Slide Wash Buffer from the wells by inverting Plate over liquid waste. Dry plate with lint free wipe. Immediately add 100  $\mu$ L of the SilverQuant Development Reagent to each well of the CSA: Simian Panel A Plate using the multichannel repeater pipette. Tap the side of the plate twice to ensure that the Development Reagent covers the entire bottom of each well of the plate.

7.4.8 Immediately start the timer and incubate for exactly 3 minutes. Place a cover (i.e. the lid of a box) over the CSA: Simian Panel A Plate to protect it from light.

7.4.9 Obtain a squirt bottle filled with fresh ultra-pure water and place next to liquid waste container.


## 7.5 Final Rinse

7.5.1 When the incubation time expires, invert the CSA: Simian Panel A Plate to remove the Development Reagent from the Plate into a proper chemical waste container and immediately fill the wells with ultrapure water using the squirt bottle. Remove water by inverting plate over sink or liquid waste.

7.5.2 Repeat the water flush twice to ensure all the Development Reagent is rinsed out.

7.5.3 Dry the CSA: Simian Panel A Plate by either using a plate centrifuge (inverting plate over paper towel and gently spin down the plate) or by letting air dry on the benchtop.

7.5.4 Empty any unused Development Reagent into a chemical waste container.

	<b>CSA: Simian Panel A</b> (Product Number 12-1212) <b>User Protocol</b>	<b>Literature Number</b>  <b>L756 27June2018</b>	<b>Page</b>  8 of 9
---	--	--	---------------------------

7.5.5 Scan and analyze the CSA: Simian Panel A Plate using the template designated in the Certificate of Analysis from the kit.

## 8.0 Ordering Information

Telephone: +1.608.561.8730

Email: [orders@intuitivebio.com](mailto:orders@intuitivebio.com) or [support@intuitivebio.com](mailto:support@intuitivebio.com)

Website: [www.intuitivebio.com](http://www.intuitivebio.com)

Colony Surveillance Assay™ and Plate™ are trademarks of Intuitive Biosciences, Inc. Madison, WI USA.

AthenaQuant® and SilverQuant® are registered trademarks of Intuitive Biosciences, Inc.

This product uses SilverQuant® technology available exclusively from Intuitive Biosciences, Inc. This product and/or the use of this product may be covered by one or more patents of EPPENDORF AG, including, but not restricted to, the following: US Patent #7,321,829 and European Patent #1179180B1.


Intuitive Biosciences' thin nitrocellulose protein microarray slide is covered by several US and foreign patents, including US Patent #6,861,251 and #7,235,307. Other US and international patents pending.

© 2018, Intuitive Biosciences, Inc. All rights reserved.

### For Research Use Only

PURCHASER SHALL USE THE PRODUCTS PURCHASED HEREUNDER (the "Products") SOLELY FOR THE PURPOSE OF CONDUCTING INTERNAL RESEARCH AT ITS ORGANIZATION ("RESEARCH"). Purchaser will not sell, transfer, disclose or otherwise provide access to the Products to any third party. Purchaser agrees that Purchaser shall not have the right to authorize any third party to use or sell any Products or derivatives thereof. Unless a license has been executed between Purchaser and Intuitive Biosciences, Inc. explicitly providing otherwise, Purchaser will not: (i) reformulate or create derivatives of the Products; or (ii) use the Products for providing services to a third party (e.g., screening or profiling); (iii) use the Products in a diagnostic process; (iv) use the Products in a quality control or quality assurance process for the manufacture of a product for sale; or (v) use the products as a component of a kit.



	<b>CSA: Simian Panel A</b> (Product Number 12-1212) <b>User Protocol</b>	<b>Literature Number</b>  <b>L756 27June2018</b>	<b>Page</b>  9 of 9
---	--	--	---------------------------

## 9.0 Appendix A: Troubleshooting

**Problem:** Weak Signal

**Suggested Causes & Solutions:**

1. Incorrect assay temperature – Reaction must occur at 18- 30°C for optimal results.
2. Protein degradation – use freshly prepared samples.
3. Slow addition of the Development Reagent – immediately add the Development Reagent to reaction tube, and cap without hesitation.
4. Incorrect assay incubation time – follow protocol for proper incubation times.

**Problem:** High Background

**Suggested Causes & Solutions:**

1. SilverQuant chromogenic reagents were exposed to light for an extended period - SilverQuant Reagents A and B should have minimal exposure to direct light. Seal the plate immediately after the Development Reagent is added to the wells.

**Problem:** No signal from detection controls

**Suggested Causes & Solutions:**

1. A step in the protocol was skipped or a reagent was mishandled.
2. If a low signal is seen in the positive controls, the anti-simian IgG gold conjugate solution was possibly missing or mishandled.

**Problem:** Heterogeneous Background

**Suggested Causes & Solutions:**

1. Washing/Drying artifact – Salts in the wash buffer may leave “streaks” in the array image. Briefly rinse wells again with purified water and immediately dry.
2. Dust may adhere to the well after it has been dried. It may be necessary blow/wipe off any dust that may have settled into a well.